

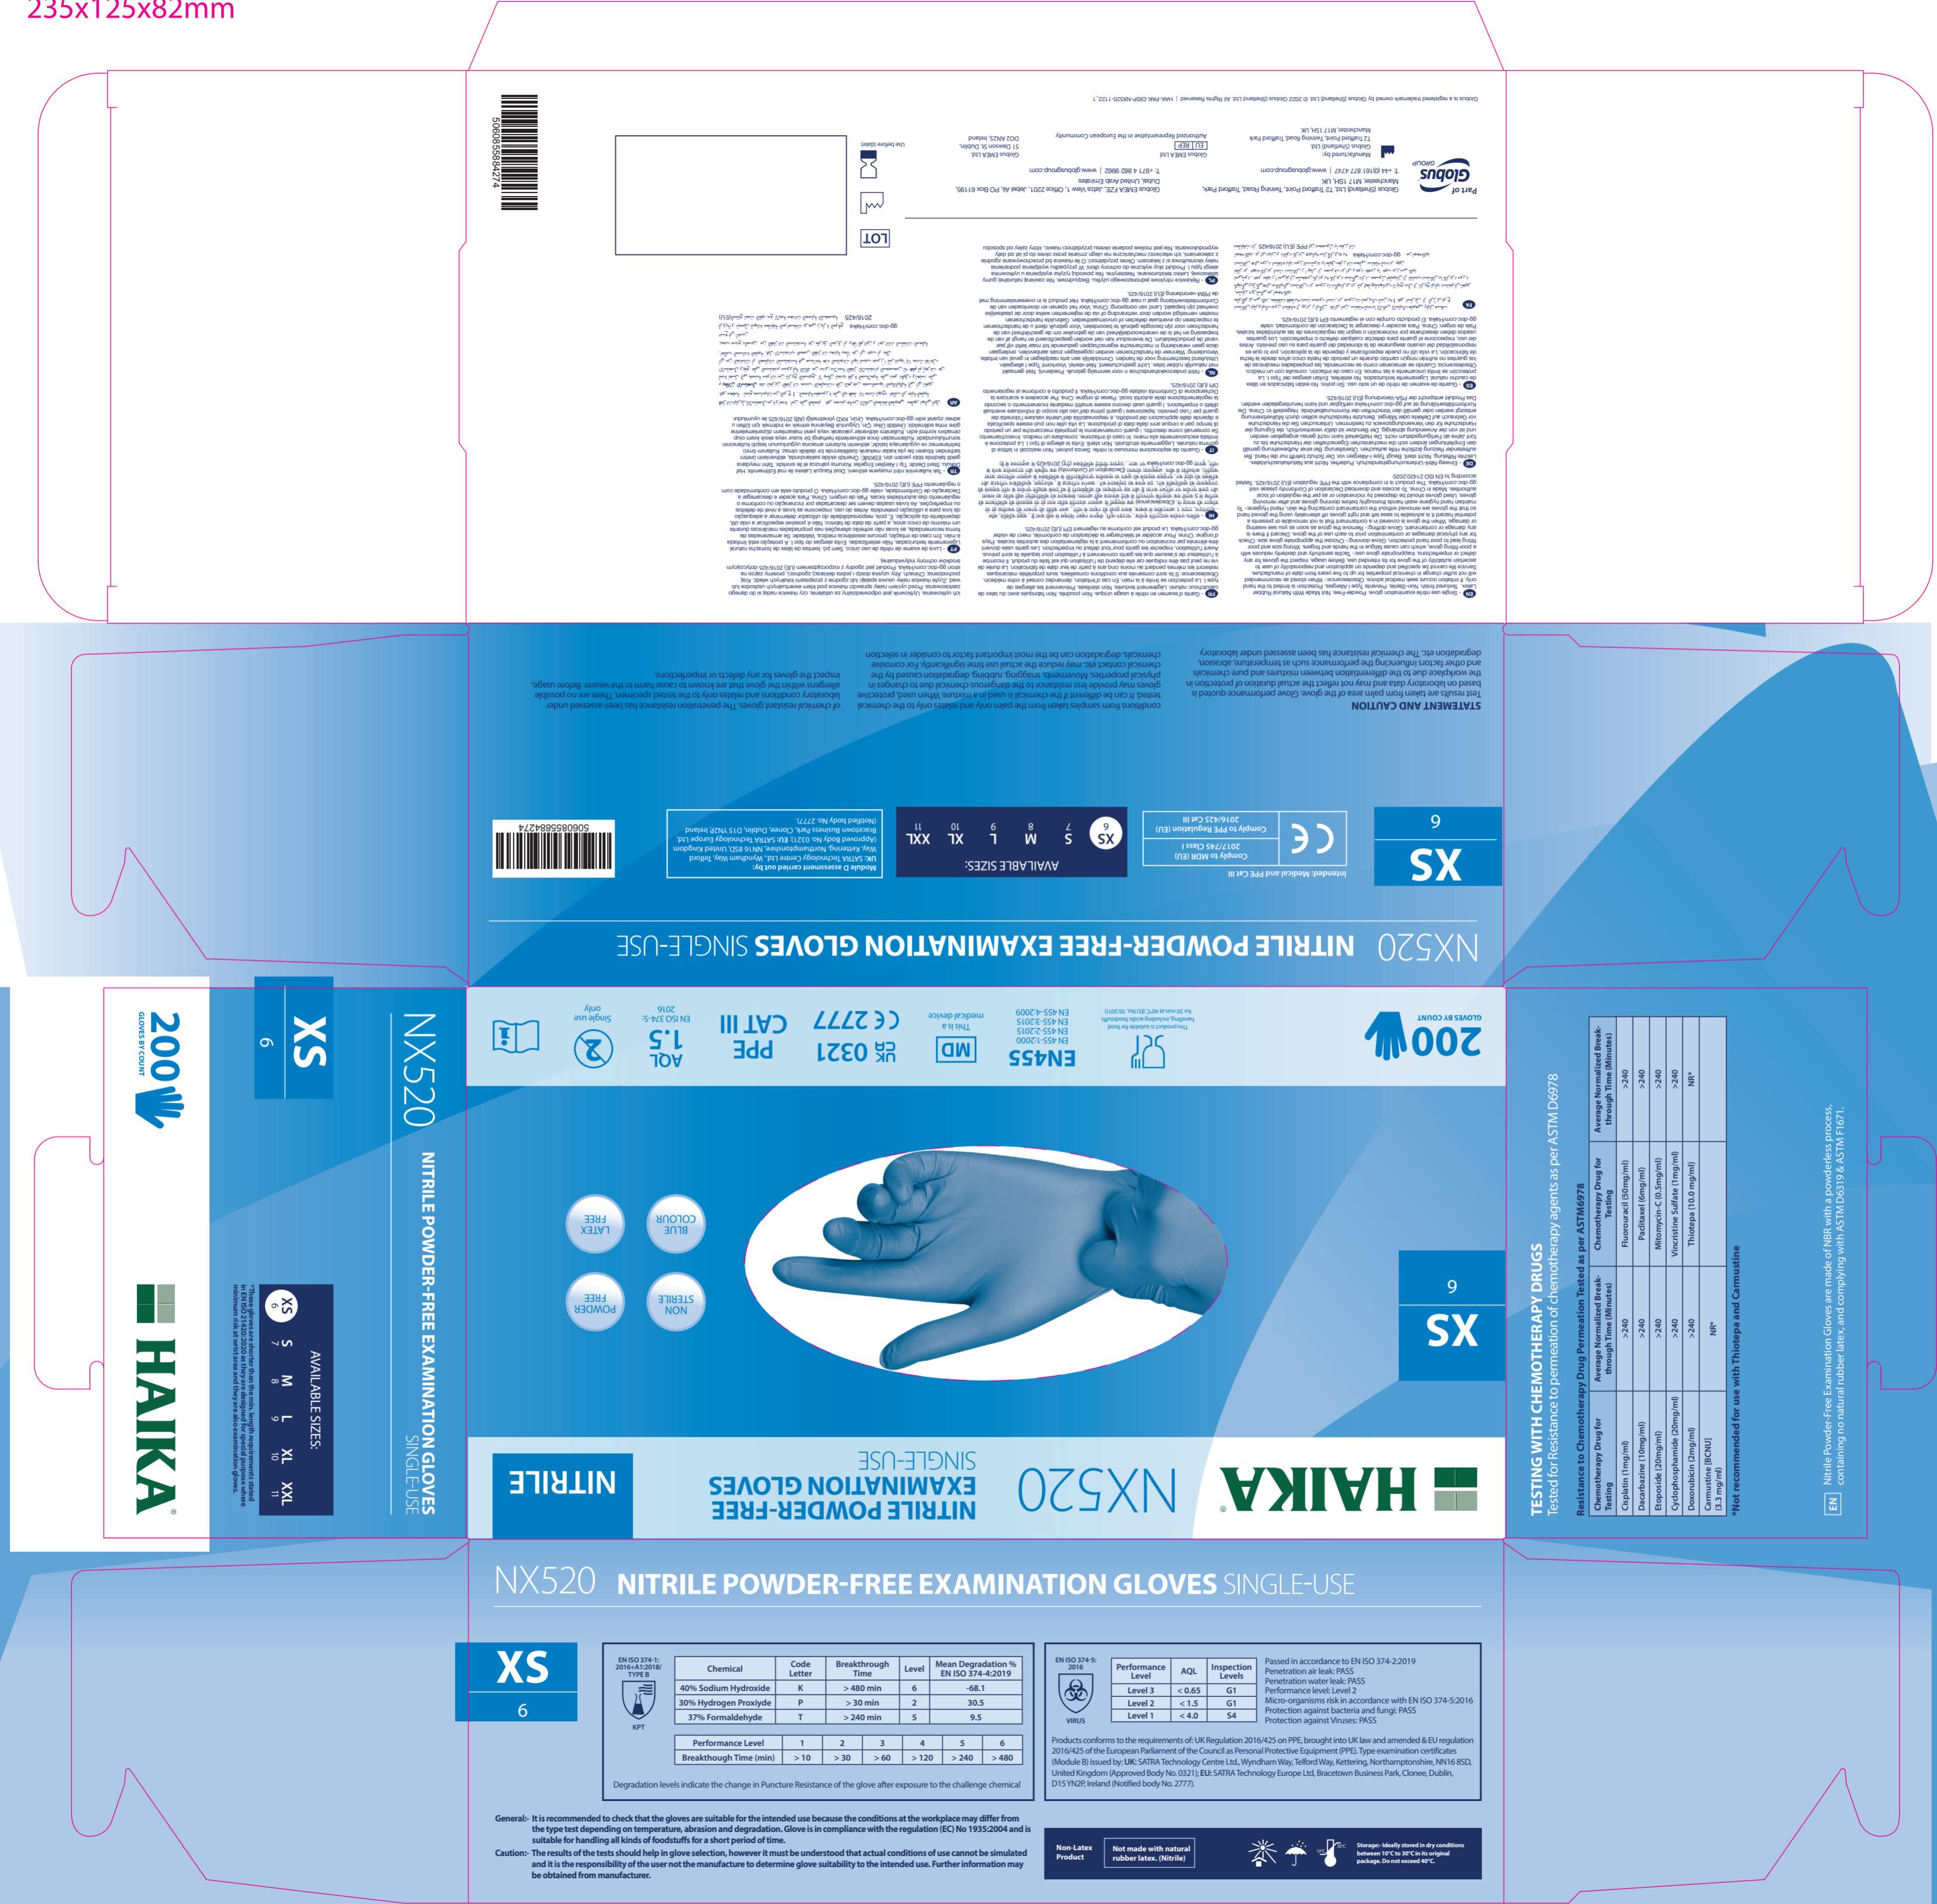


235x125x82mm

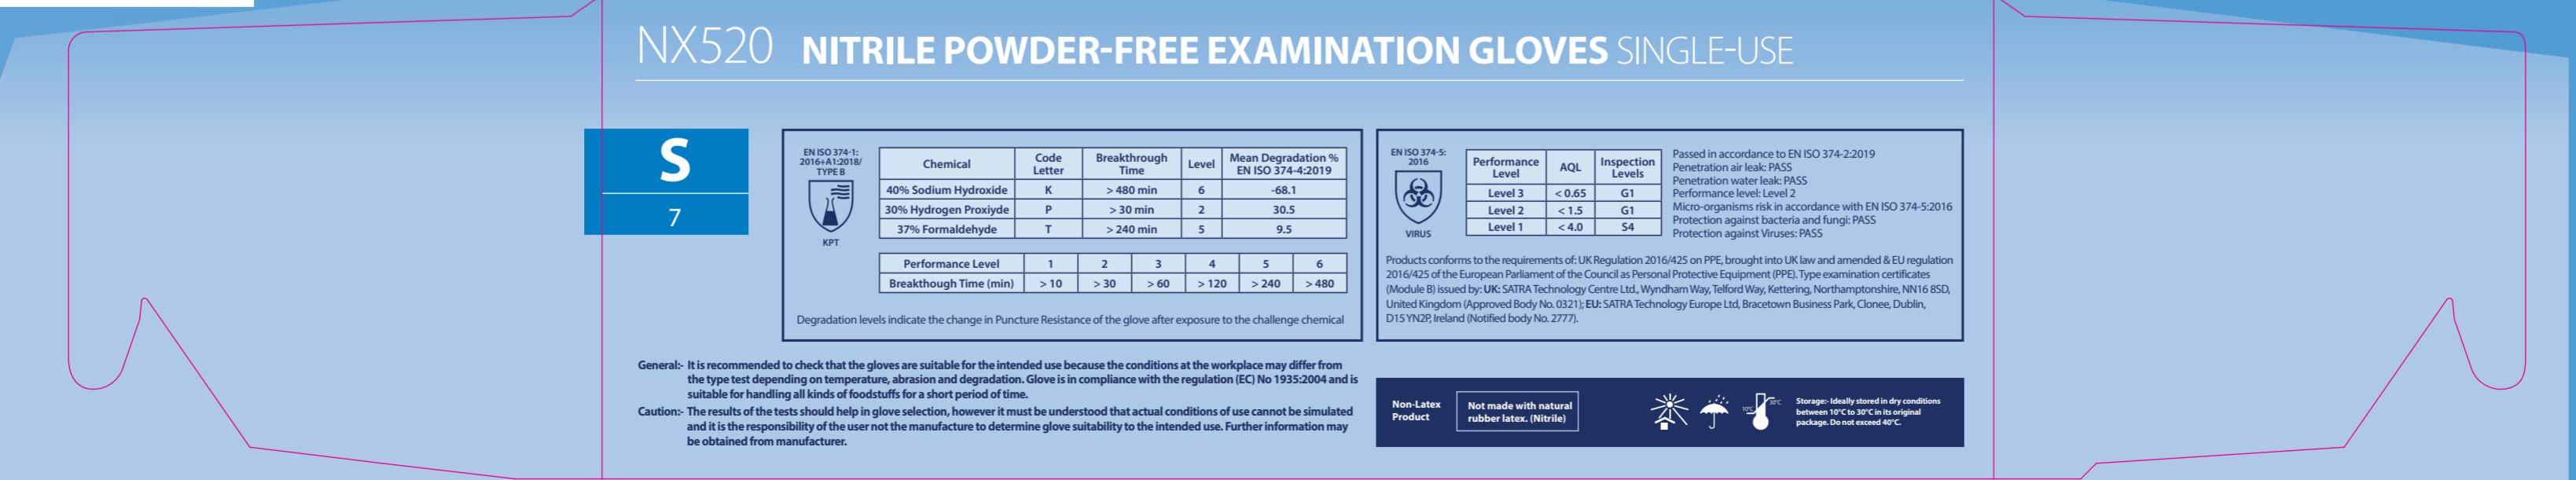

235x125x82mm

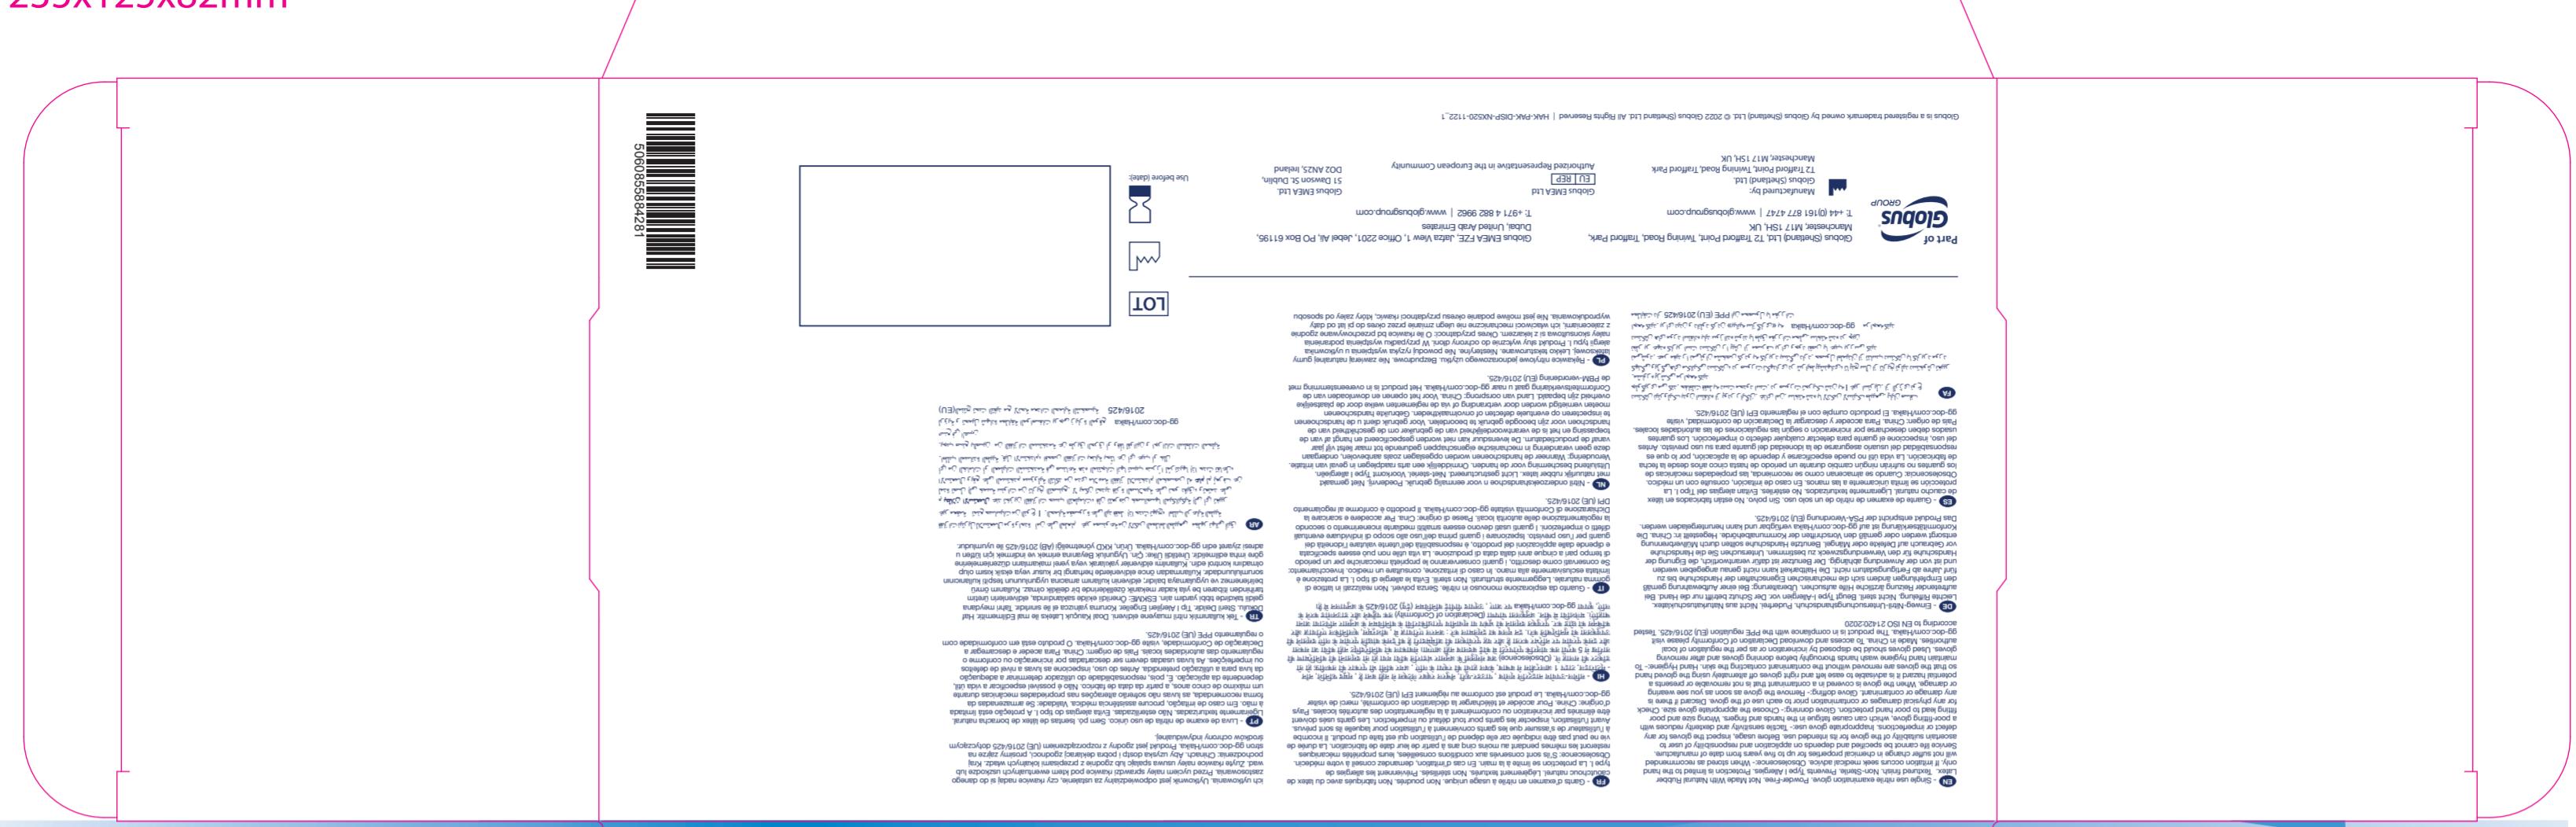

235x125x82mm

**NX520 NITRILE POWDER-FREE EXAMINATION GLOVES SINGLE-USE**

**M 8**

**General:** It is recommended to check that the gloves are suitable for the intended use because the conditions at the workplace may differ from the type test depending on temperature, abrasion and degradation. Glove is in compliance with the regulation (EC) No 2035/2004 and is suitable for handling all kinds of foodstuffs for a short period of time.

**Caution:** The results of the tests should help in glove selection, however it must be understood that actual conditions of use cannot be simulated and it is the responsibility of the user not the manufacturer to determine glove suitability to the intended use. Further information may be obtained from manufacturer.

**EN ISO 374-1: 2016+A1:2018/ TYPE B**

Chemical	Code Letter	Breakthrough Time	Level	Mean Degradation % EN ISO 374-2:2019
40% Sodium Hydroxide	K	> 480 min	6	-68.1
30% Hydrogen Peroxide	P	> 30 min	2	30.5
37% Formaldehyde	T	> 240 min	5	9.5

Performance Level	1	2	3	4	5	6
Breakthrough Time (min)	> 10	> 30	> 60	> 120	> 240	> 480

Degradation levels indicate the change in Puncture Resistance of the glove after exposure to the challenge chemical

**EN ISO 374-5: 2016**

Performance Level	AQL	Inspection Levels
Level 3	< 0.65	G1
Level 2	< 1.5	G1
Level 1	< 4.0	S4

Passed in accordance to EN ISO 374-2:2019  
Penetration water leak: PASS  
Performance level: Level 2  
Micro-organisms risk in accordance with EN ISO 374-5:2016  
Protection against bacteria and fungi: PASS  
Protection against viruses: PASS

Products conform to the requirements of UK Regulation 2016/425 on PPE brought into UK law and amended & EU regulation 2016/425 of the European Parliament of the Council as Personal Protective Equipment (PPE). Type examination certificates (Module B) issued by: UK: SATRA Technology Centre Ltd, Wyndham Way, Telford Way, Kettering, Northamptonshire NN16 8SD, United Kingdom (Approved Body No. 0321); EU: SATRA Technology Europe Ltd, Bracebridge Business Park, Clonee, Dublin, D15 YN2P; Ireland (Notified body No. 2777).

**Non-Latex Product** **Not made with natural rubber latex. (Nitrile)** **Storage:** Ideally stored in dry conditions away from heat and direct sunlight. Store in a cool, dry place in original package. Do not exceed 40°C.


**TESTING WITH CHEMOTHERAPY DRUGS** Tested for Resistance to permeation of chemotherapy agents as per ASTM D6978

Chemotherapy Drug for Testing	Average Normalized Break-through Time (Minutes)	Chemotherapy Drug for Testing	Average Normalized Break-through Time (Minutes)
Cisplatin (1mg/ml)	>240	Fluorouracil (50mg/ml)	>240
Diclofenac (10mg/ml)	>240	Paclitaxel (6mg/ml)	>240
Etoposide (20mg/ml)	>240	Mitomycin-C (5mg/ml)	>240
Cyclophosphamide (20mg/ml)	>240	Vincristine Sulfate (1mg/ml)	>240
Doxorubicin (2mg/ml)	>240	Thiotepa (10.0 mg/ml)	>240
Carmustine (6.3 mg/ml)	NR*		


\*Not recommended for use with Thiotepa and Carmustine

**EN** Nitrile Powder-Free Examination Gloves are made of NBR with a powderless process.

235x125x82mm

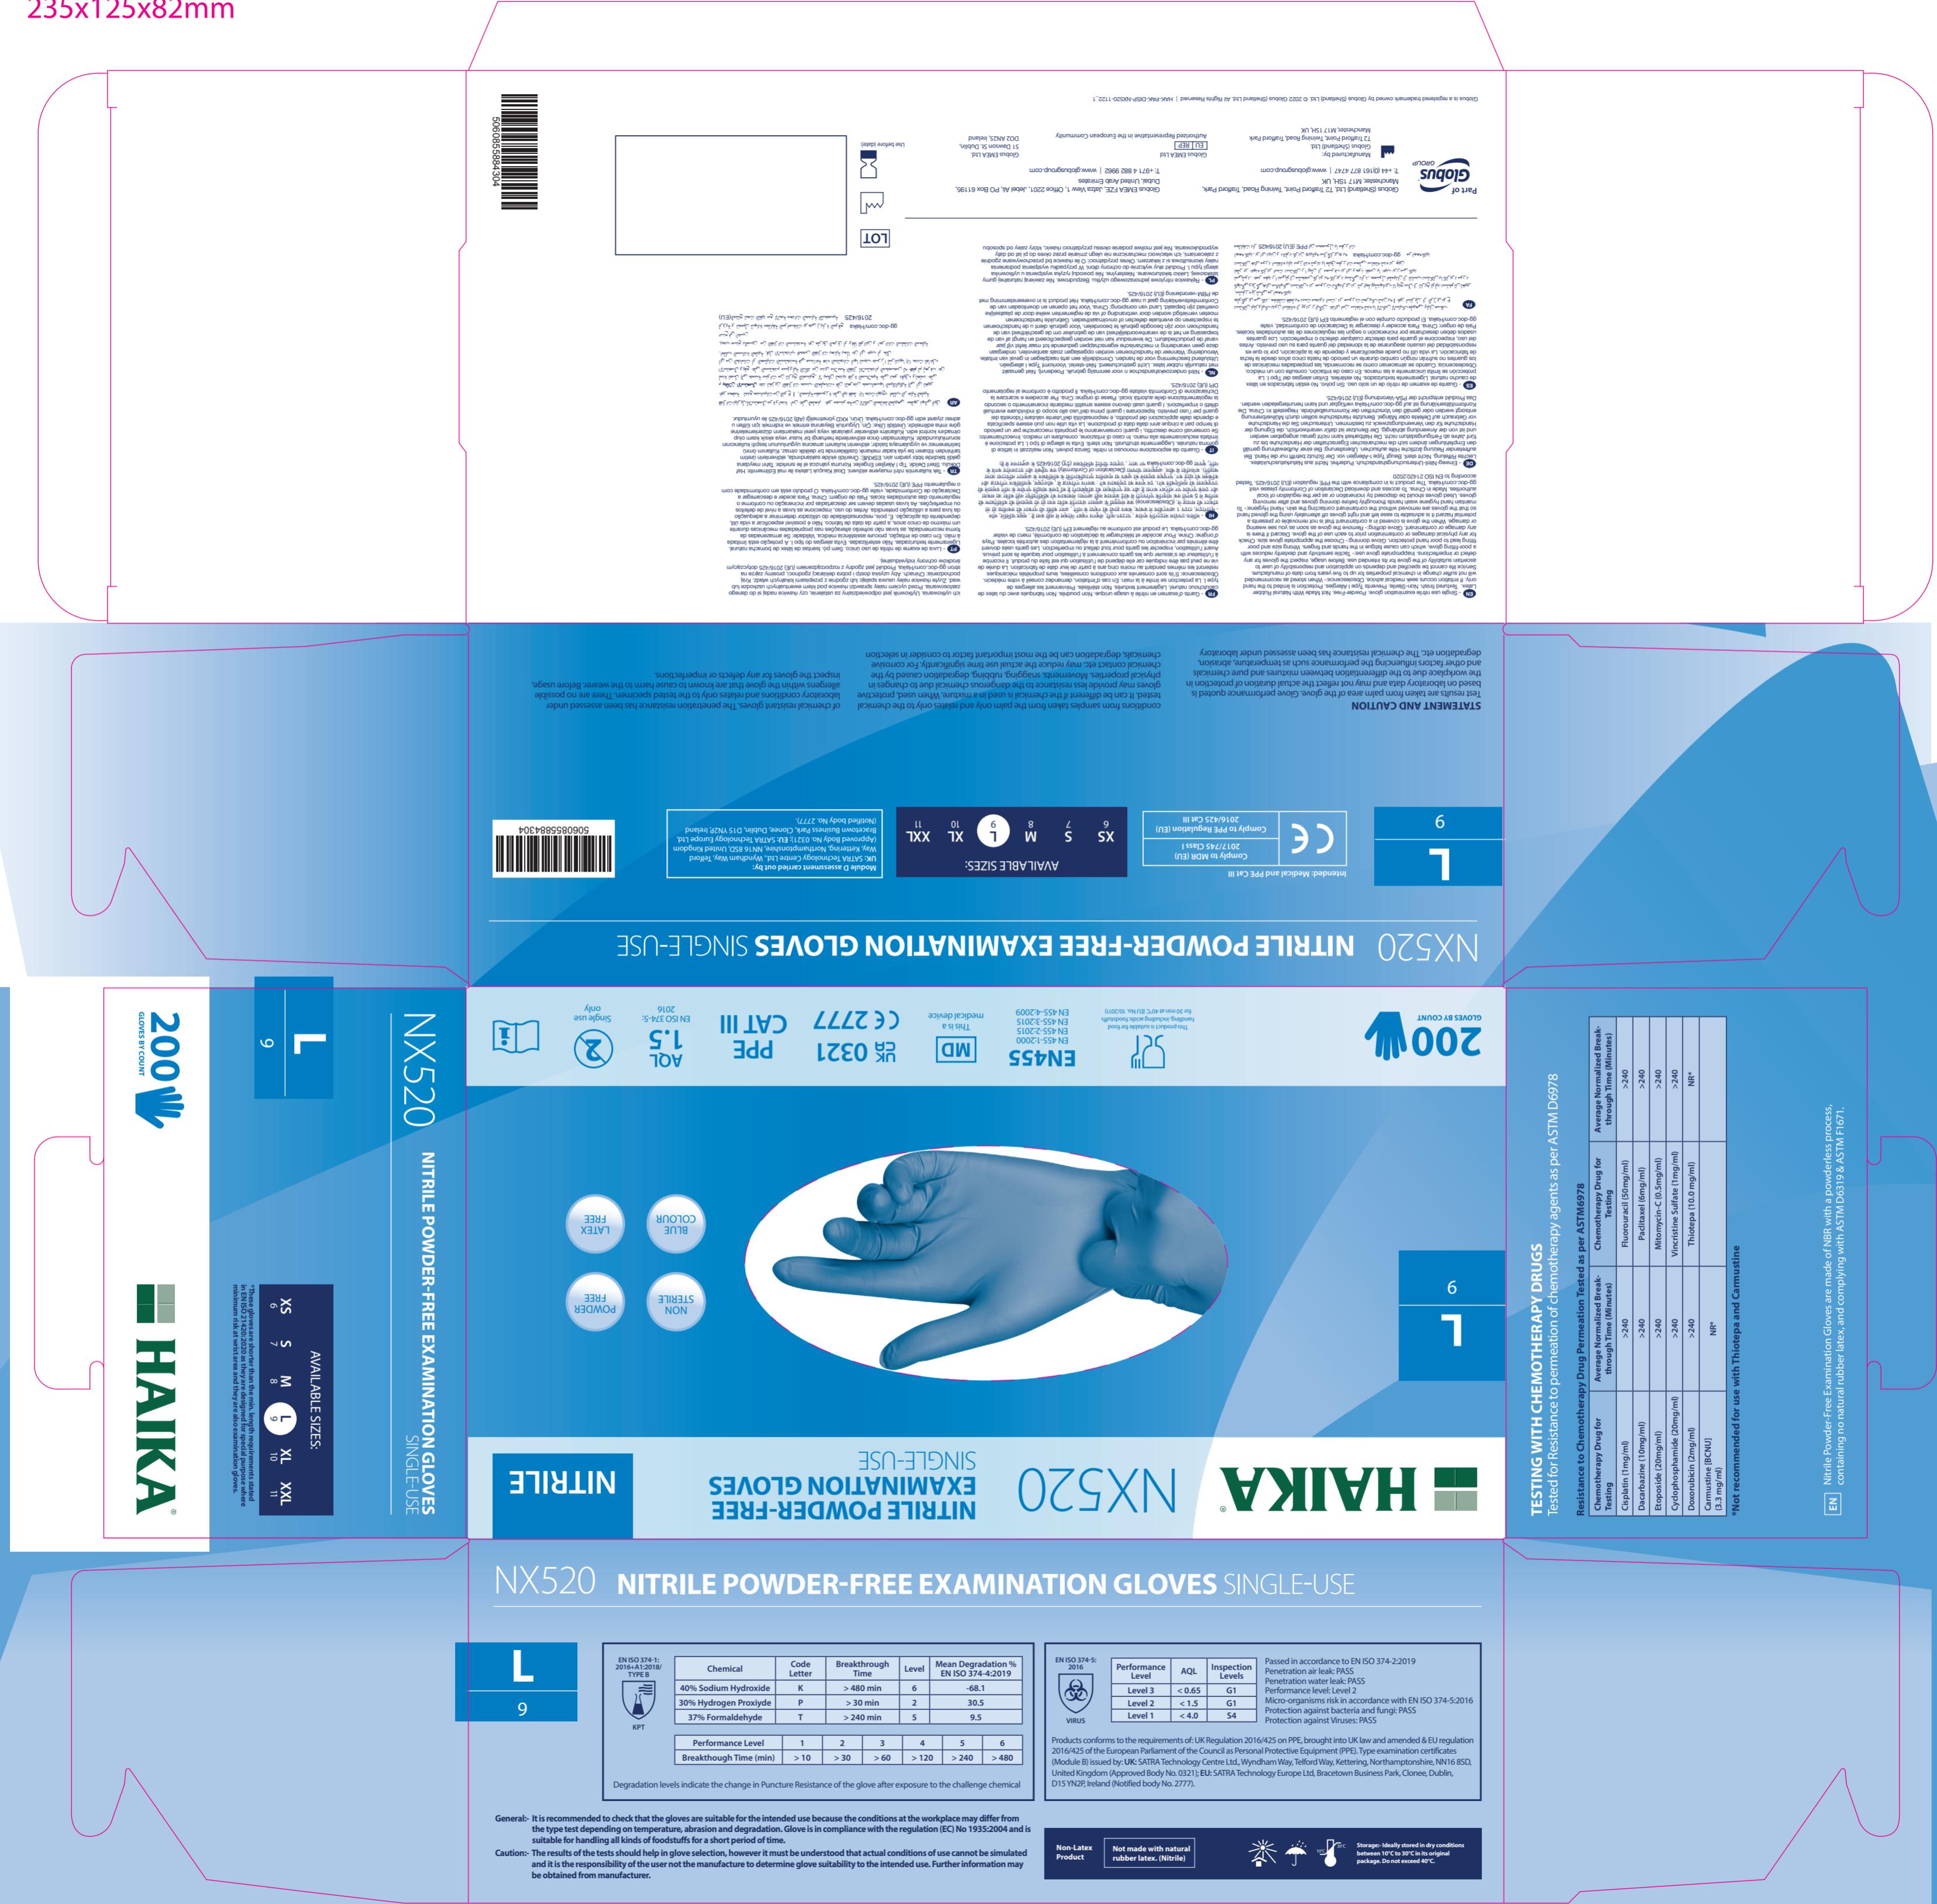

235x125x82mm

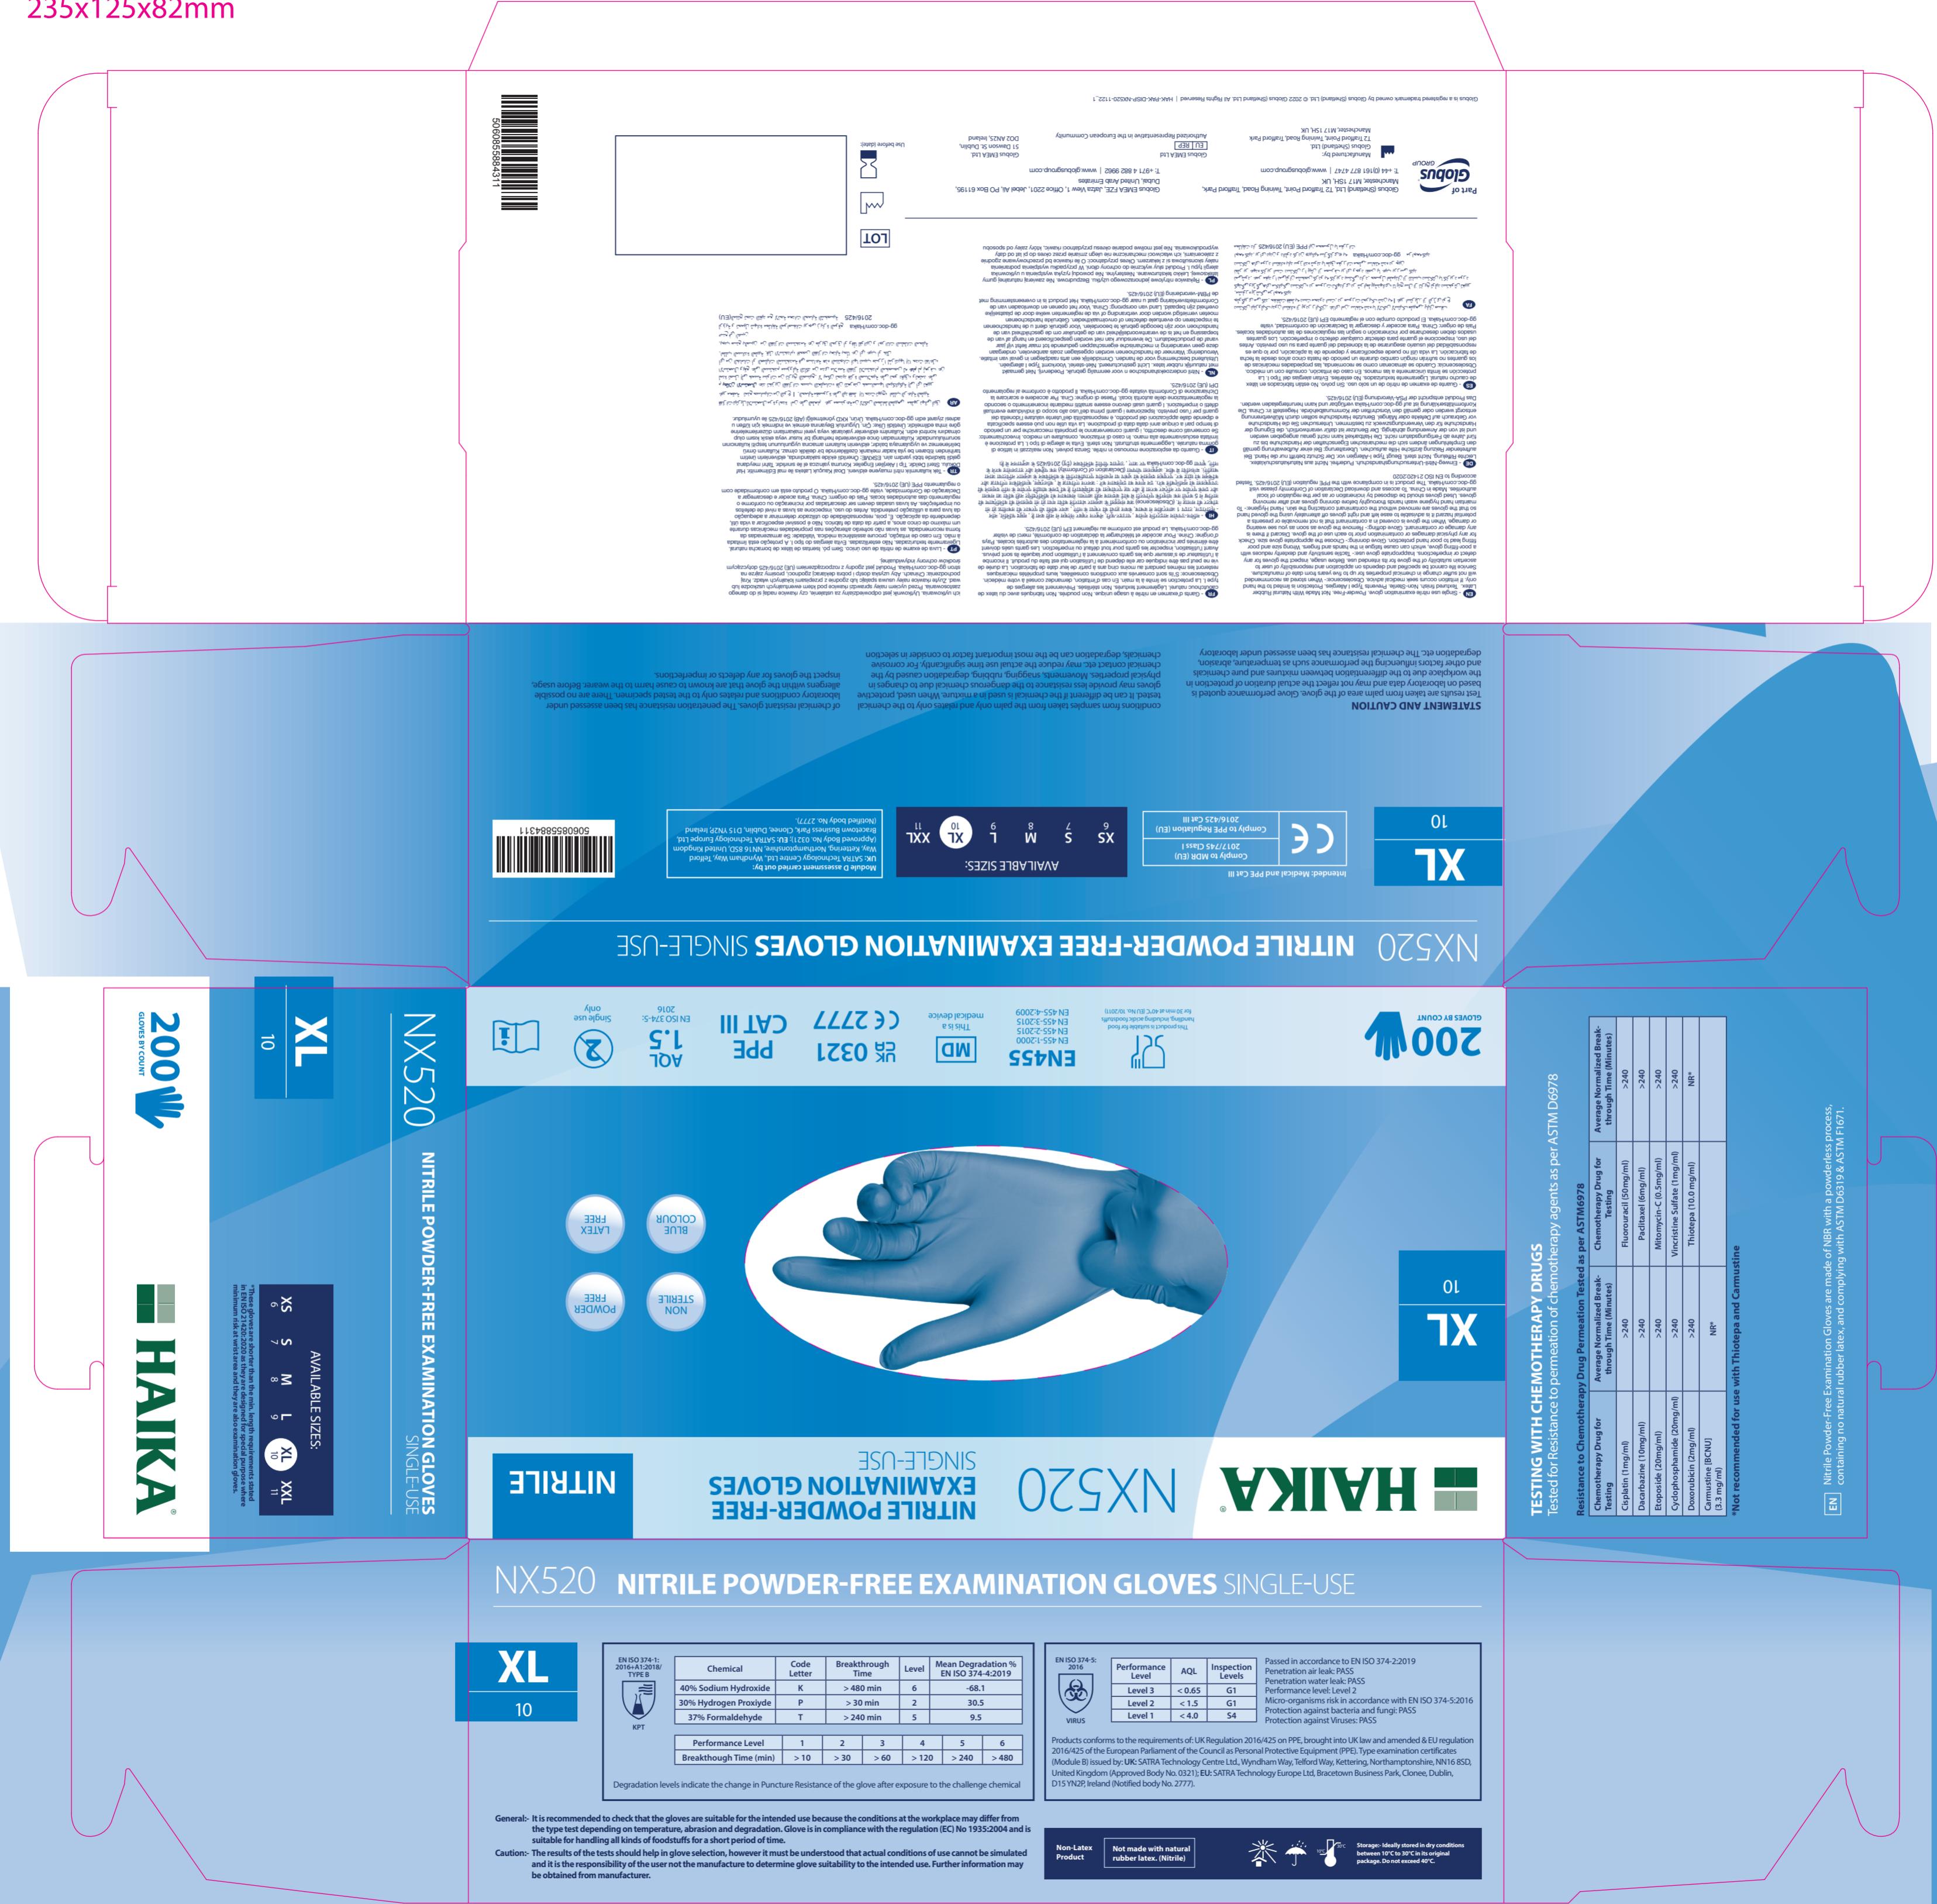

235x125x82mm

